




Igenity[®] Tissue Sample Instructions

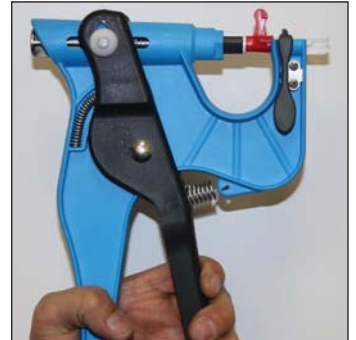

1. Remove a TSU punch from the packaging. Punches should be assembled as one piece; if they have come apart, reassemble. Open the tube retainer at the base of the applicator by pushing the retainer clip.

2. Insert the punch into the applicator. Release the clip to lock punch into the device. Carefully squeeze the applicator handles together, guiding the punch tip into place if necessary. When the gun bolt rests flush against the red plastic clip, release the handle.



3. Remove the red plastic clip by pulling it outward. Be careful as the metal cutter above the clip is very sharp. Ensure the applicator is loaded with an unused punch (if the red plunger is visible, the punch is used and should be replaced with one that is unused).

4. Slide the applicator over the animal's ear and position the metal cutter one inch from the edge of the ear, making sure to avoid any obvious veins or ridges. Squeeze handles together to take a sample and then release to free the ear. Try to do this in one swift, fluid motion.



5. Remove the punch from the applicator and check that sampling has been successful. If not, discard the sample and proceed with a new punch. Remove the used cutter from the applicator by pulling the handles apart. Discard carefully as the cutter is very sharp.



Neogen: GeneSeek Operations • 4131 N. 48th Street, Lincoln, NE 68504
877-443-6489 • www.neogen.com/genomics • igenity.support@neogen.com

